

Monoclonal Antibody to CD45, FITC conjugated (CD45 FITC)

Cat.No. ED7018

1. Intended purpose

The reagent CD45 FITC permits identification and enumeration of cell populations expressing human CD45 antigen in whole blood using flow cytometry.

2. Test principle

This test is based on specific binding of monoclonal antibody to the antigenic determinant expressed on the surface of leukocytes. The monoclonal antibody is labeled with fluorochrome which is excited via laser beam from a flow cytometer during analysis. Subsequent emission of light from fluorochromes of each cell is collected and analyzed by a flow cytometer. The fluorescence intensity differences enable separation of cell subsets based on expression of analyzed antigen. Specific staining of blood cells is performed by incubation of blood samples with the reagent followed by a lysis of red blood cells. Afterwards, unaffected leukocytes are subjected to analysis by a flow cytometer.

3. Reagents provided

The reagent contains mouse monoclonal antibody against human CD45 antigen (clone MEM-28) which was purified by affinity chromatography and labeled with Fluorescein isothiocyanate (FITC). The labeled antibody is diluted in an optimal concentration in stabilizing phosphate buffered saline (PBS) solution containing 15mM sodium azide. The content of a vial (2 ml) is sufficient for 100 tests.

Product specification

Content	100 tests, 2 ml
Usage	20 µl per test
Specificity	Human CD45
Clone	MEM-28
Isotype	Mouse IgG1
Fluorochrome	FITC
λ excitation	488 nm
Emission maximum	525 nm

4. Materials required but not provided

Test tubes for blood staining (e.g. 12 × 75 mm)
Commercial lysing solution
Phosphate buffered saline (PBS)
Isotype control antibody (mouse IgG1 FITC)

5. Equipment required

Automatic pipettes with disposable tips
Vortex mixer
Centrifuge
Flow cytometer with excitation laser 488 nm and proper filters

6. Storage and handling

Store the vial at 2-8°C. Keep away from sunlight. Do not freeze. Do not aliquot. Expiration date is stated on a vial label and on outer packaging.

7. Warnings, precautions and limitations of use

- Intended for In Vitro Diagnostic use in laboratories outside USA and Canada. This reagent is in conformity with the European Directive 98/79/EC.
- Do not use reagent after expiration date.
- Avoid reagent contamination.
- Avoid prolonged exposure to light.
- The content of the vial must not freeze.
- Any non-performance of staining protocol may produce false results.
- The reagent contains sodium azide (NaN₃) which is highly toxic in pure form. However, the concentration in the reagent (15mM) is not considered as hazardous. When disposing the reagent, flush the sink with a large volume of water.
- Blood samples are considered as potentially infectious and must be handled with care. Avoid all contact of the sample with the skin, eyes and mucosa.
- In case of hyperleukocytose sample, it is recommended to dilute blood sample with PBS to obtain leukocyte density approximately 5 × 10⁶ leukocytes/ml.
- Blood samples from abnormal patients may exhibit abnormal values of positive cells.
- Data may be incorrectly interpreted if fluorescent signals were compensated wrongly or if gates were positioned

- inaccurately.
- Flow cytometer may produce false results if the device has not been aligned and maintained appropriately.
- Red blood cells from abnormal patients may be resistant to lysis using lysing solutions.
- Blood samples should be stained and analyzed within 24 hours from the blood collection.

8. Specimen

Use the peripheral human blood in a sterile tube with an anticoagulant (Heparin or EDTA). Blood must be stored at room temperature.

9. Procedure


Staining protocol

- Add 20 µl of CD45 FITC reagent to a test tube, and the necessary amount of isotype control to a control tube.
- Add 100 µl of blood sample to each tube. Vortex the tubes.
- Incubate tubes for 15 - 20 minutes at room temperature in the dark.
- Perform lysis of red cells using lysing solution. It is recommended to use a commercial lysing solution containing formaldehyde as a fixative. Follow the instructions of the lysing solution manufacturer.
- Centrifuge tubes for 5 minutes at 300 g.
- Remove supernatant and resuspend pellet with 3 - 4 ml of PBS.
- Centrifuge tubes for 5 minutes at 300 g.
- Remove supernatant and resuspend pellet with 0.3 - 0.5 ml of PBS.
- Analyze samples immediately using flow cytometer or store samples at 2-8°C in the dark and analyze within 24 hours provided that cells were fixed.

Flow Cytometric Analysis

Analyze the sample stained with CD45 FITC using a flow cytometer. Visualize recorded data using appropriate plot such as side-scatter (SSC) versus FITC intensity as shown in figure 1. All leukocytes are bright (CD45+), nonleukocytes (debris, erythrocytes, platelets, etc.) are dim (CD45-). Set suitable gates for analysis.

Fig. 1: Leukocytes stained with CD45 FITC reagent

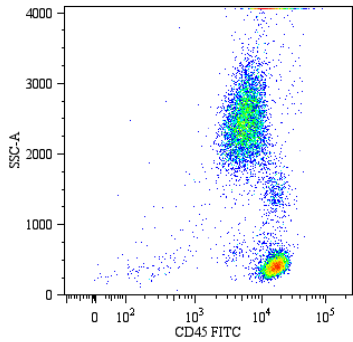

10. Analytical performance

Specificity

The antibody MEM-28 reacts with all alternative forms of human CD45 phosphotyrosine phosphatase (Leukocyte Common Antigen), a 180-220 kDa single chain type I trans-membrane protein expressed at high level on all cells of hematopoietic origin, except from erythrocytes and platelets. The monoclonal antibody MEM-28 was assigned to CD45 during the Human Leukocyte Differentiation Antigen workshop (HLDA3 WS Code: NL 833a).

11. Clinical performance

Expected values

N/A

12. References

- Guttinger M et al. (1992) CD45 phosphotyrosine phosphatase and p56lck protein tyrosine kinase: a functional complex crucial in T cell signal transduction. Int Immunol. 4: 1325-30
- Stover DR et al. (1991) Protein-tyrosine-phosphatase CD45 is phosphorylated transiently on tyrosine upon activation of Jurkat T cells. Proc Natl Acad Sci USA 88: 7704-7707
- Taetle R et al. (1991) Regulation of CD45 expression in human leukemia cells. Leukemia 5: 309-314
- Nakano A et al. (1990) Expression of leukocyte common antigen (cd45) on various human leukemia/lymphoma cell lines. Acta Pathol Jpn. 40: 107-115
- Yamada A et al. (1990) Effect of activation of protein kinase C on CD45 isoform expression and CD45 protein tyrosine phosphatase activity in T cells. Eur J Immunol. 20: 1655-60
- Bazil V et al. (1989) Sialic acid-dependent epitopes of CD45 molecules of restricted cellular

expression. Immunogenetics 29: 202-5

Horejsi V et al. (1988) Monoclonal antibodies against human leucocyte antigens. II. Antibodies against CD45 (T200), CD3 (T3), CD43, CD10 (CALLA), transferrin receptor (T9), a novel broadly expressed 18-kDa antigen (MEM-43) and a novel antigen of restricted expression (MEM-74). Folia Biol (Praha). 34: 23-34

Leukocyte Typing IV., Knapp W. et al. (Eds.), Oxford University Press (1989).

Leukocyte Typing III., McMichael A. J. et al (Eds.), Oxford University Press (1987).

13. Manufacturer

EXBIO Praha, a.s.
Nad Safinou II 341
25250 Vestec
Czech Republic

info@exbio.cz
technical@exbio.cz
orders@exbio.cz
www.exbio.cz

14. Trademarks

N/A

15. Revision History

- Version 1, ED7018_IFU_v1
Initial Release
- Version 2, ED7018_IFU_v2
Merging three language mutations into one document.
Intended use section was changed - "The reagent could be used in various antibody panels for multi-parameter flow cytometry analyses." - removed.
Staining protocol section was changed - step 5 - "(e.g. ADG-LYSE produced by AN DER GRUB, Cat. No. GAS-003)." - removed.
Limitations section was changed - "Results obtained in different laboratories may vary. Each laboratory should establish a normal range of positive cells using its own test conditions." - removed.
- Version 3, ED7018_IFU_v3
The address was changed: "Nad Safinou II 341."
- Version 4, ED7018_IFU_v4
Precautions section was changed - "Intended for professional use only." - removed. "Intended for In Vitro Diagnostic use in laboratories outside USA and Canada. This CE-IVD reagent is in conformity with the European In Vitro Diagnostic Medical Device Directive 98/79/EC." - added.
- Version 5, ED7018_IFU_v5
Reagent provided section was changed: text "stabilizing" added, "solution" - added and "0.2% (w/v) high-grade protease free Bovine Serum Albumin (BSA) as a stabilizing agent" - removed.
- Version 6, ED7018_IFU_v6
The company logo changed. IFU layout changed. "Keep away from sunlight." - added. Postal code changed: "25250 Vestec".



Monoclonal Antibody to CD45, FITC conjugated (CD45 FITC)

100 tests | Cat.No. **ED7018**



Instructions for Use

Version: ED7018_IFU_v6_EN

Date of Issue: 07-10-2020

EN

Symbols



Catalogue number



Batch code



Use-by date



Temperature limits



Keep away from sunlight



In vitro diagnostic medical device



CE marking of conformity



Consult instructions for use



Manufacturer

The product is intended for In Vitro Diagnostic Use. In vivo diagnostic or therapeutic applications are strictly forbidden.

Products shall not be used for resale or transfer to third parties either as a stand-alone product or as a manufacture component of another product without written consent of EXBIO Praha, a.s. EXBIO Praha, a.s. will not be held responsible for patent infringement or any other violations of intellectual property rights that may occur with the use of the products. Orders for all products are accepted subject to the Term and Conditions available at www.exbio.cz. EXBIO, EXBIO Logo, and all other trademarks are property of EXBIO Praha, a.s..